

Healand Labs
www.healandlabs.co.uk


Sample received: **07/30/26**
Analysis conducted: **08/11/26**

Product:	Selank 15mg + Semax 15mg
Batch:	HL262905
Appearance:	Lyophilized peptide vial

Qualitative and quantitative chemical analysis by RP-HPLC with UV detection
Endotoxin count by kinetic chromogenic LAL assay

Results

Analyte	Specification	Result	
Selank	15mg	15.38mg	Conforms
Semax	15mg	16.73mg	+11.5%
Blend purity	> 98%	99.103%	Conforms
Endotoxins:	< 80 EU/vial	< 5 EU/vial	Conforms
Metals:	< 50 ppb	< 50 ppb	Conforms

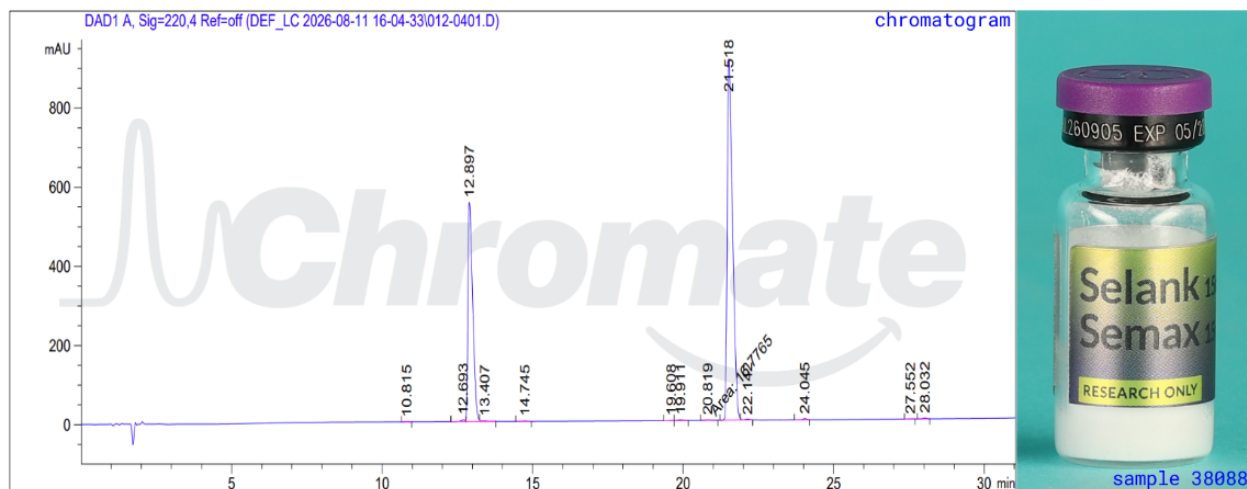

Lucas Weber
Lucas Weber
Principal Chemist

COA #38088
access code HEALAND14CCM
chromate.org/verify
produced 08/11/26

